
BioCLIA[®] Autoimmune Calibrator Set

PCNA

PCNA Assay Calibrators

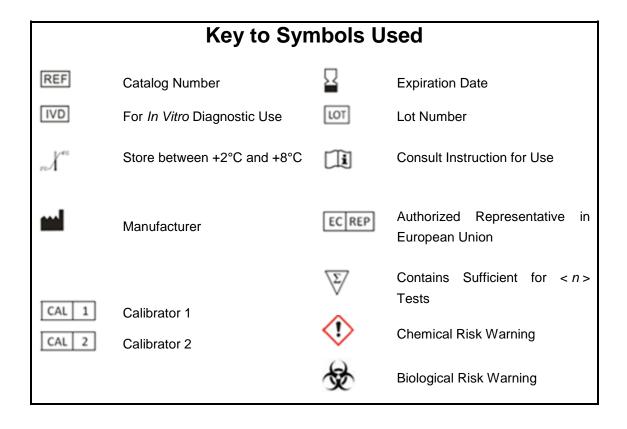

BioCLIA® Autoimmune Calibrator

Set, PCNA

Intended Use

The BioCLIA Autoimmune Calibrator Set, PCNA is intended for the calibration of the BioCLIA PCNA performed on the BioCLIA® 1200 and BioCLIA® 6500.

Catalog Numbers

MY00208 (2 X 1 mL) My00259 (4 X 1 mL)

Summary and Explanation

Anti-nuclear antibodies (ANAs) are a class of auto-antibodies with different binding affinities specific to different nuclear antigens. Generally, ANAs include extractable nuclear antigen (ENA) antibodies and un-extractable nuclear antigen antibodie. 1 Determination of ANAs has significant correlation to the diagnosis of Sharp Syndrome, Systemic Lupus Erythematosus (SLE), Sjogren's Syndrome, progressive systemic sclerosis, polymyositis/dermatomyositis, overlap syndrome, and limited types of progressive systemic sclerosis (CREST syndrome).

Proliferating cell nuclear antigen (PCNA) is a DNA clamp that acts as a processivity factor for DNA polymerase δ in eukaryotic cells and is essential for replication. Antibodies against proliferating cell nuclear antigen (PCNA, a kind of ANA marker) or monoclonal antibody termed Ki-67 can be used for grading of different neoplasms, e.g. astrocytoma. They can be of diagnostic and prognostic value. Imaging of the nuclear distribution of PCNA (via antibody labeling) can be used to distinguish between early, mid and late S phase of the cell cycle.

Materials supplied

- PCNA Calibrator 1 A tube contains 1mL, ready to use reagent. Control contains human antibodies to PCNA in stabilizers and preservatives. Preservatives: 0.0015% < Proclin 300 < 0.6% PCNA CAL 1
- PCNA Calibrator 2 A tube contains 1mL, ready to use reagent. Control contains human antibodies to PCNA in stabilizers and preservatives. Preservatives: 0.0015% < Proclin 300 < 0.6% PCNA CAL 2

Target value information is indicated in the 2D barcode localized in each kit.

Warnings and Precautions

The human derived material in this product was tested by FDA approved methods and found nonreactive for Hepatitis B Surface Antigen (HBsAg), Anti-HCV and HIV 1/2 antibodies. Handle as if potentially infectious. 5 Avoid contacting with skin and eyes. Do not empty into drains. Wear suitable protective clothing.

Precautions:



Human serum is added in the calibrators.



Proclin 300 is added in the calibrators at concentration between 0.0015% - 0.6%.

- The product is for in vitro diagnostic use only.
- Do not use any calibrators beyond their expiration dates. Do not mix calibrators from different lots unless specified.
- · Instructions must be carefully followed for using and storing of calibrators. Any modification in procedure may interfere with the results. Calibrators and contaminated vials must be handled strictly following safety guidelines or rules of biological hazards to ensure the users' and environmental safety.
- Calibrators contain chemical and biological components. Avoid ingesting or splashing onto skin and mucous membrane. If direct contact with calibrators happens, rinse immediately the contact surface with plenty of water and see a doctor if necessary.

Storage Conditions

The kit is stable until the expiration date, if stored and handled as directed. Routine store the kit in refrigerator (2-8°C). Once a calibrator tube is opened, it is good for a total of 15 times, no more than 2 hours per time when kept uncapped, onboard the instrument, after which the reagent must be discarded. Three freeze-thaw cycles before testing has no effect on the kit reagents.

Assay Procedure

Note that, for obtaining optimal performance, it is important to perform all routine maintenance procedures as defined in the BioCLIA®1200 and BioCLIA® 6500 User Manual.

See the BioCLIA® 1200 and BioCLIA® 6500 User Manual for preparation, setup, dilutions, adjustment, assay and quality control procedures.

Traceability

The reported values were determined over multiple runs on the BioCLIA® 1200 and BioCLIA® 6500 using specific lots of reagents against an in-house standard. PCNA results are reported in RU/mL which is interpreted from relative light unit (RLU). Method comparison test showed good sensitivity and specificity of tested assay.

Limitations

This product is designed as calibrators for monitoring the performance of the BioCLIA PCNA. These calibrators are subjected to the limitations of the assay system. Deviations may indicate problems with one or more components in the test system.

References

- Tan EM. Autoantibodies to nuclear antigens (ANA): their immunobiology and medicine. Advances in Immunology 1982;33:167-240.
- Schönenberger F, Deutzmann A, Ferrandomay E, Merhof D. Discrimination of cell cycle phases in PCNA-immunolabeled cells. BMC Bioinformatics 2015;16:1-10.
- 3. Herce HD, Rajan M, Lättig-Tünnemann G, Fillies M, Cardoso MC. A novel cell permeable DNA replication and repair marker. Nucleus 2014;5:590-600.
- 4. Wang S-C. PCNA: a silent housekeeper or a potential therapeutic target? Trends in pharmacological sciences 2014;35:178-86.
- 5. Richmond JY, Mckinney RW. Biosafety in microbiological and biomedical laboratories: U.S.GPO. 1999.





HOB Biotech Group Co., Ltd

C6 Building, No. 218 Xinghu Road, Suzhou Industrial Park, Suzhou, Jiangsu, 215123, China

REGISTRANT/MANUFACTURE: HOB Biotech Group

Co., Ltd

ADDRESS/LOCATION:

C6 Building, No. 218 Xinghu Road, Suzhou Industrial Park, Suzhou, Jiangsu, 215123 China

CONTACT INFORMATION: TEL (+86)512-69561996

Fax (+86)512-62956652

WEBSITE: www.hob-biotech.com

CUSTOMER SERVICE: HOB Biotech Group Co., Ltd CUSTOMER SERVICE CONTACT: TEL (+86)4008601202



EUROPE REPRESENTATIVE: Emergo Europe

ADDRESS/LOCATION:

Prinsessegracht 20, 2514 AP The Hague, The

Netherlands

Technical Assistance

For technical assistance, contact your National Distributor.

17th April 2019

Revision 9